


Differences in Therapeutic Dosage Range by Manufacturer (Biphasic)



Medtronic Philosophy:

“The clinician should set the dose – not the manufacturer.”

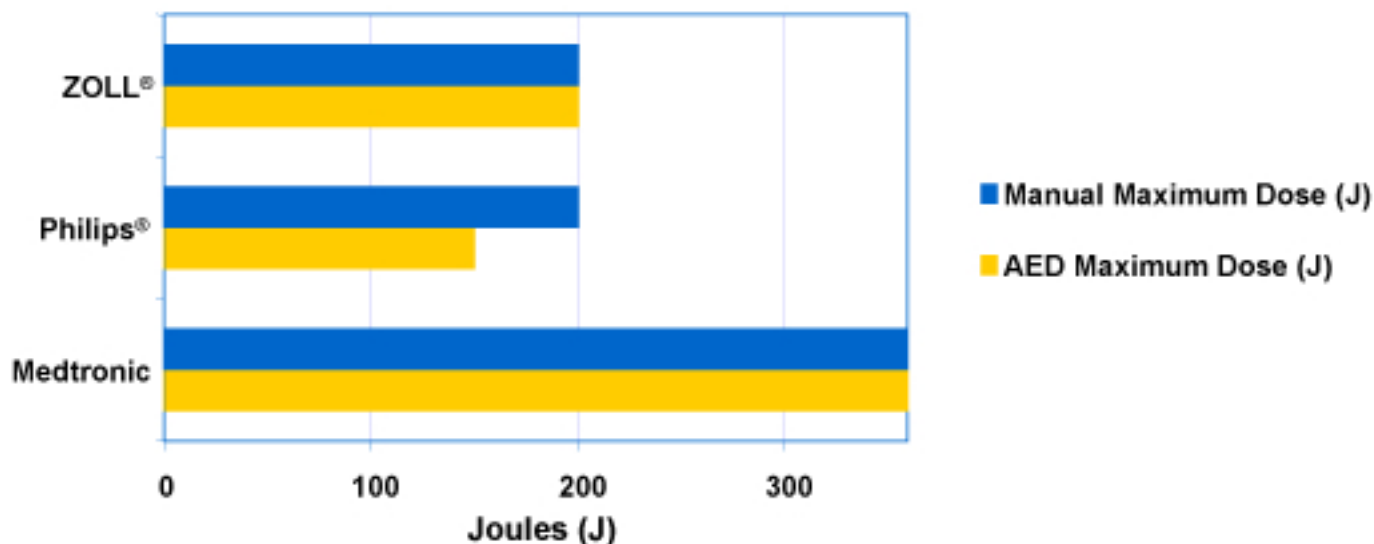