

Noninvasive Pacing

An Evidence-Based Approach to Clinical Claims

Some suppliers of external pacing devices continue to claim their devices have superior performance. It is important to evaluate these claims in light of the highest standards of clinical evidence:

- Independent studies with prospective, randomized design
- Studies that match patients in each comparison arm by demographics and medical condition


It is also important to avoid cross-study comparisons involving disparate study designs and endpoints.

THE DEFINITIVE STUDY ON PACING EFFICACY

Physio-Control devices use a pacing impulse duration of 20ms while ZOLL uses a pacing impulse duration of 40ms. A study by Falk et al.¹ demonstrates there is no statistically significant difference between Physio-Control and ZOLL pacing technologies in terms of capture thresholds, capture rates or pain. Falk concludes “there is no benefit in increasing the pacing impulse duration, at least >20 ms.”

This is the definitive clinical comparison of these pacing technologies—providing the highest level of clinical evidence available. It’s a head-to-head, randomized comparison with matched patient arms.

Falk Study Pacing Capture Thresholds

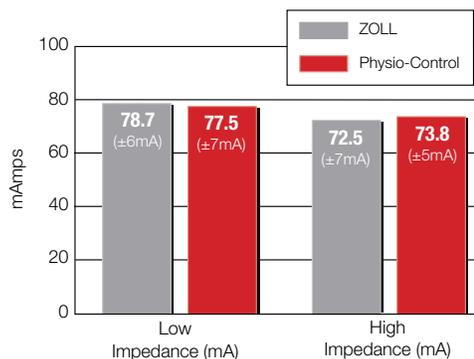

PATIENT COMFORT

Competing claims have also been made about differences in patient comfort associated with various pacing technologies. While addressing patient comfort, Falk states, “Both devices caused an equal amount of discomfort...suggesting that the difference in pacing impulse characteristics is of no clinical significance.”¹

Anecdotal evidence about potential differences in patient comfort was supplied in a 1988 court case by a former president of ZOLL. In that case, he testified under oath that he personally had been paced with a Physio-Control device and a ZOLL device, that he could not “distinguish between the two machines,” and that “they were indistinguishable as to comfort.”²

THE PHYSIO-CONTROL POSITION

Physio-Control remains committed to operating under the highest standards of evidence when educating and informing our customers. We believe clinical claims should be thoughtfully made in order to avoid overinterpretation. At this time there are no well-designed clinical studies that support any company’s claims of superior pacing technology.

1. Falk RH, Battinelli NJ. 1993. External cardiac pacing using low impedance electrodes suitable for defibrillation: a comparative blinded study. *J Am Coll Cardiol.*; 8: 1354–1358.
2. W.D. WA 1988) ZMI Corporation v. Physio-Control Corporation, 1998. U.S. Dist. LEXIS 17280.



Physio-Control, Inc.
11811 Willows Road NE
P.O. Box 97006
Redmond, WA 98073-9706 USA
Tel 425 867 4000
Toll-Free (USA Only) 800 442 1142
Fax 425 867 4146
www.physio-control.com