


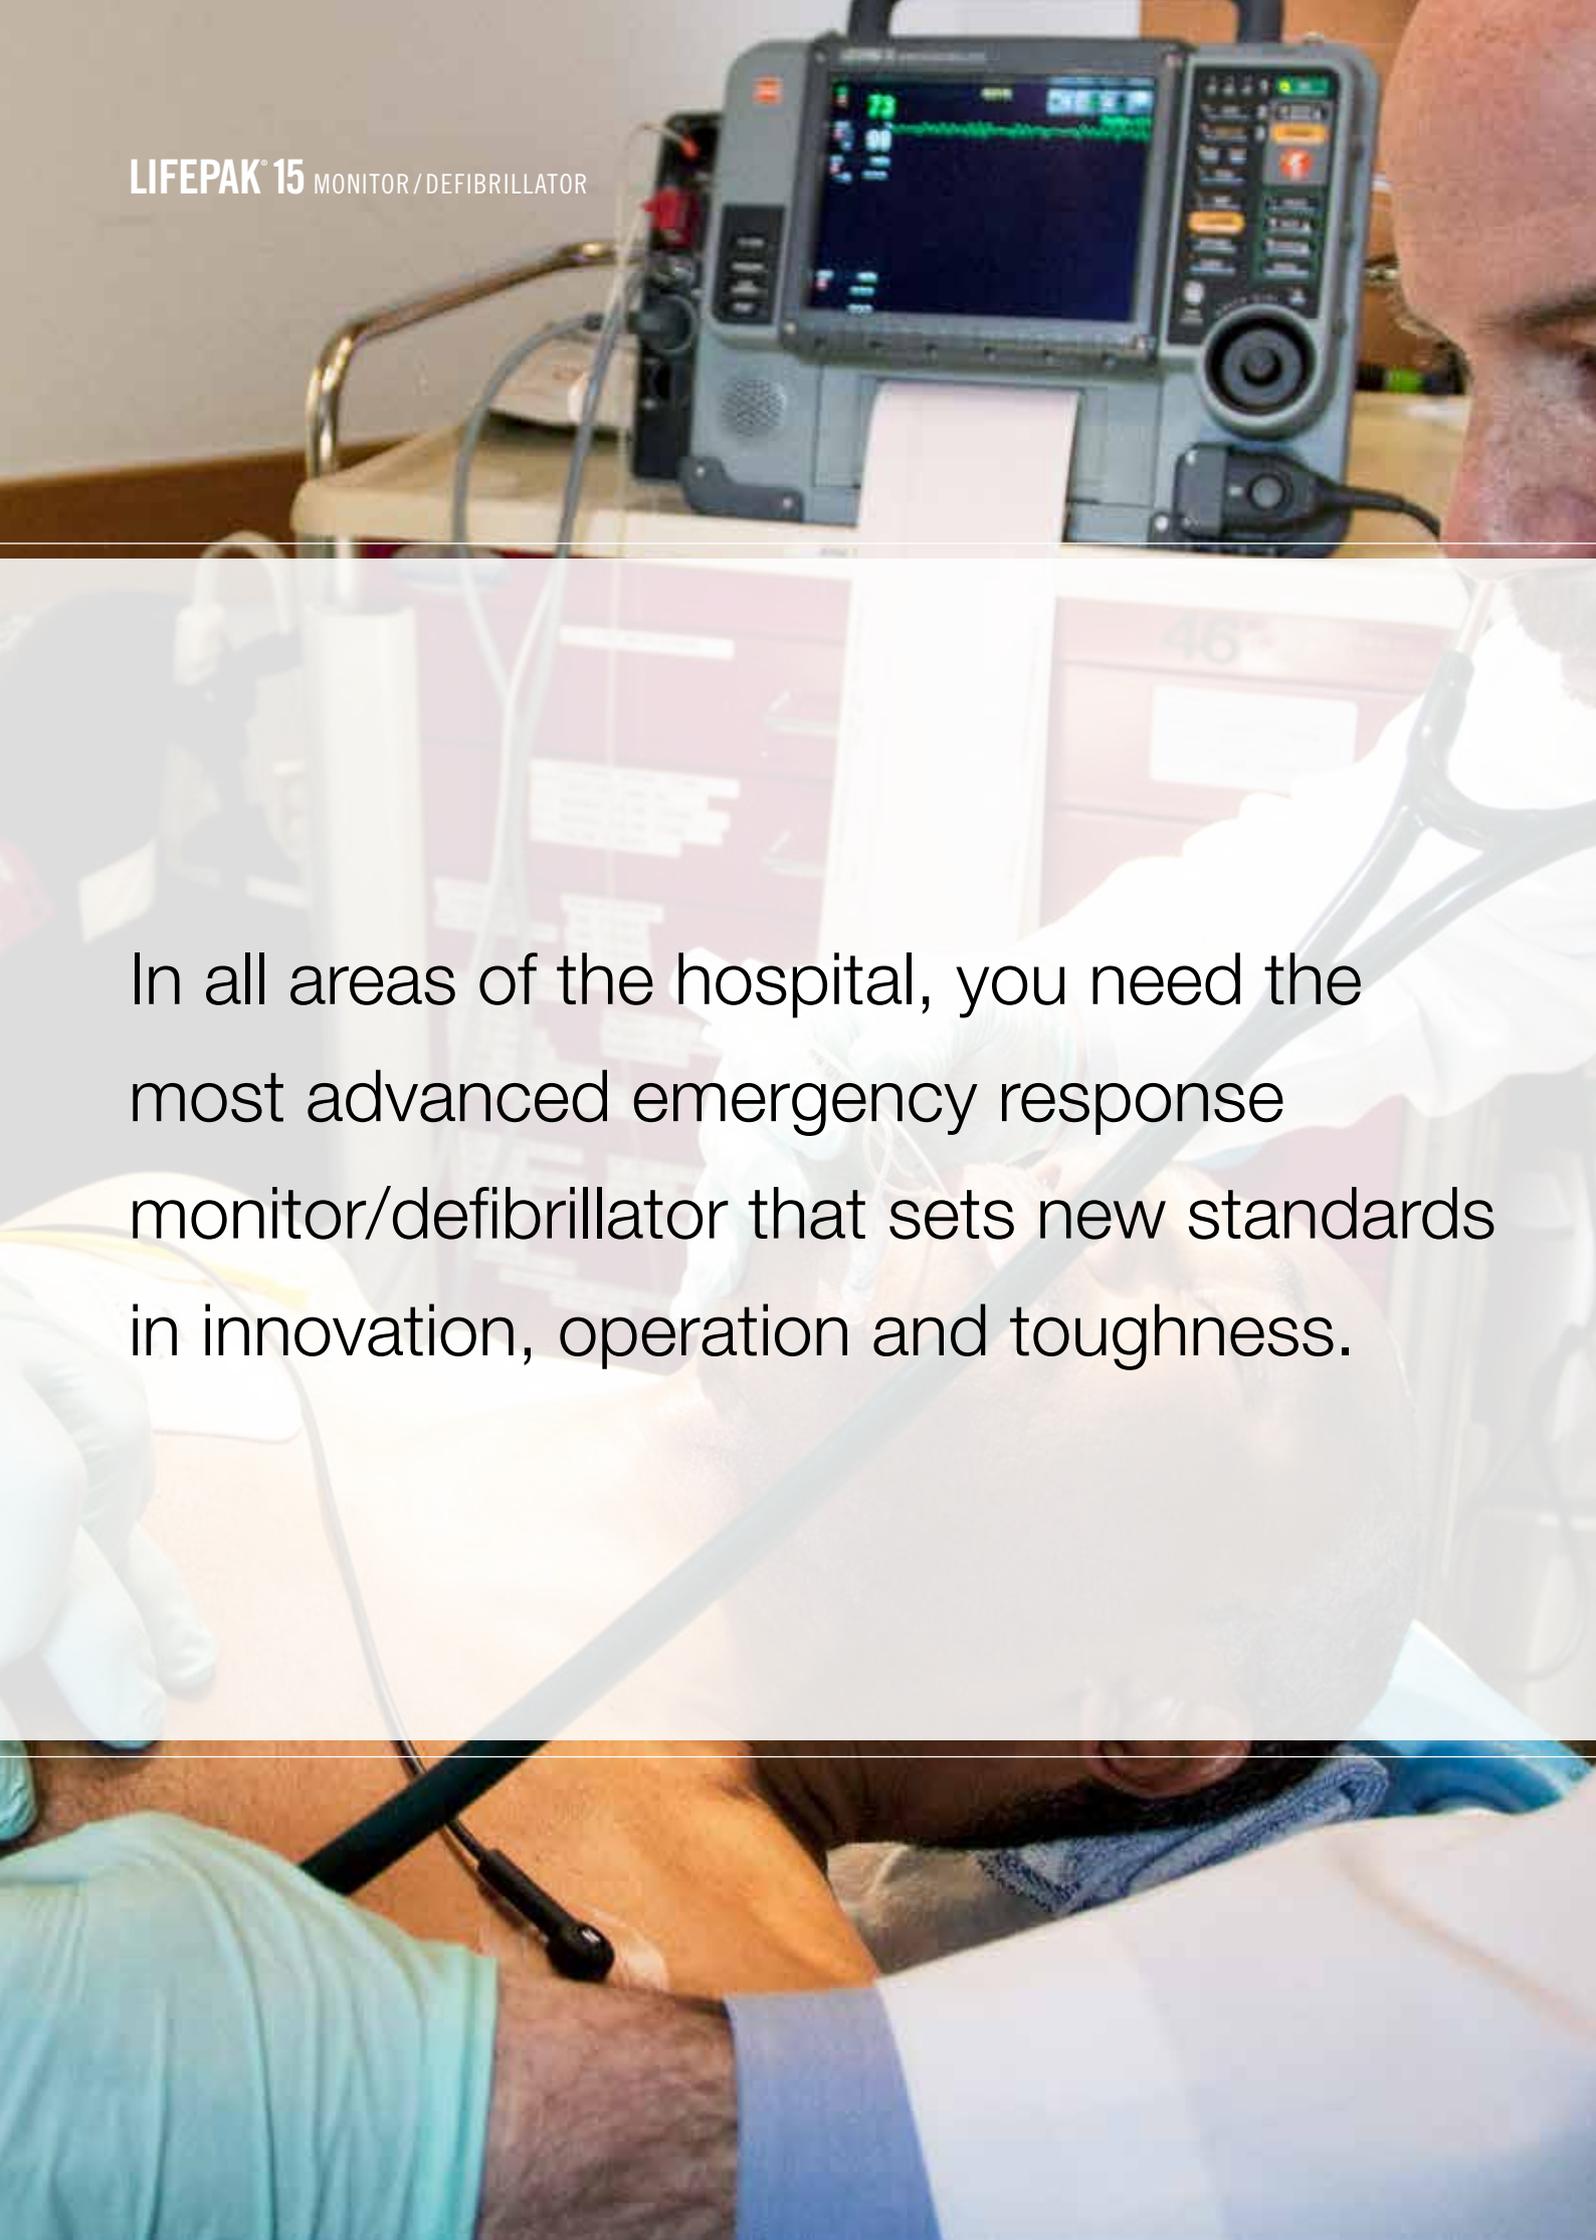

LIFEPAK® 15 MONITOR/DEFIBRILLATOR
For Hospitals

LIFEPAK[®] 15 MONITOR/DEFIBRILLATOR

A LIFEPAK 15 monitor/defibrillator is shown on a cart in a hospital room. The device has a large screen displaying vital signs, including a heart rate of 73. A paper printout is emerging from the front. In the foreground, a patient is lying in a hospital bed, partially covered by a white sheet. A stethoscope is visible around the patient's neck. The background shows a hospital room with a bed and some equipment.

In all areas of the hospital, you need the most advanced emergency response monitor/defibrillator that sets new standards in innovation, operation and toughness.



The LIFEPAK 15 monitor/defibrillator delivers.


Physio-Control defibrillators have set the standard for over 60 years, and the enhanced LIFEPAK 15 monitor raises the bar. As our most advanced emergency response monitor/defibrillator, the LIFEPAK 15 device offers sophisticated clinical technologies and operational effectiveness with a rich array of features—like the most powerful escalating energy available (up to 360J), advanced monitoring parameters, and a completely upgradable platform. At the same time, it's tough enough to stand up to your most challenging environments.

A LIFEPAK device never stands on its own—and the LIFEPAK 15 monitor is no different. Physio-Control is committed to providing complete solutions for any area of the hospital.

Our products have helped save tens of thousands of lives. We're proud to continue this work with the LIFEPAK 15 monitor/defibrillator.

The standard in clinical innovation.

The pioneer in portable defibrillation and monitoring technology, Physio-Control is committed to improving technologies and devices—such as the powerful LIFEPAK 15 monitor/defibrillator.

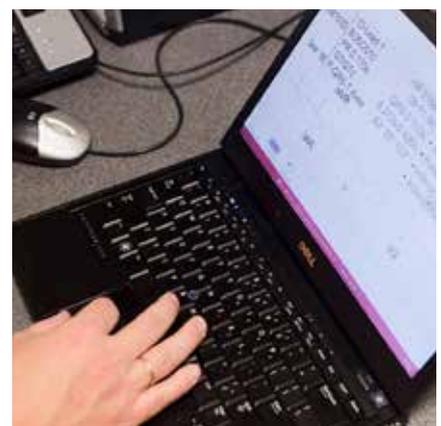

Advanced monitoring parameters

With Masimo® Rainbow® Technology, the 15 includes noninvasive monitoring of carbon monoxide, SpO₂, and methemoglobin so you can detect hard-to-diagnose conditions and improve patient care. In addition to optional NIBP and two invasive pressures, you get optional temperature monitoring with five disposable sensors—and like other data, you can include temperature in reports, download to other health information systems, or display through post event review in CODE-STAT™ software.



Advanced support for treating cardiac patients

Not only can you easily acquire a pre-medication 12-lead ECG, you can also rely on the LIFEPAK 15 monitor/defibrillator to continuously monitor all 12 leads in the background and alert you to changes using the ST-Segment Trending feature. The 15 also works seamlessly with the web-based LIFENET System, so you can automatically share critical patient data with multiple patient care teams throughout a region in real time.

Full energy up to 360 joules, for every patient who needs it

The LIFEPAK 15 monitor/defibrillator features 360J biphasic technology, which gives you the option of escalating your energy dose up to 360J for difficult-to-defibrillate patients. Why is this necessary? Recent studies have shown that refrillation is common among VF cardiac arrest patients and that defibrillation of recurring episodes of VF is increasingly difficult. A randomized controlled clinical trial shows the rate of VF termination was higher with an escalating higher energy regimen of 200J and over.¹


Proven CPR guidance and post event review

The CPR Metronome in the LIFEPAK 15 monitor uses audible prompts to guide you without distracting vocal critique. A metronome has been a feature that has demonstrated to help you perform compressions and ventilations within the recommended range of the 2010 ERC Guidelines. Post-event review of CPR data and delivering feedback to the team has been shown to be effective in improving CPR quality in both hospital and out-of-hospital.^{2,3,4} And by transmitting code data directly to CODE-STAT Data Review software, QA/QI personnel can review CPR statistics and provide training and feedback where it is most needed.



LIFEPAK[®] 15 MONITOR/DEFIBRILLATOR



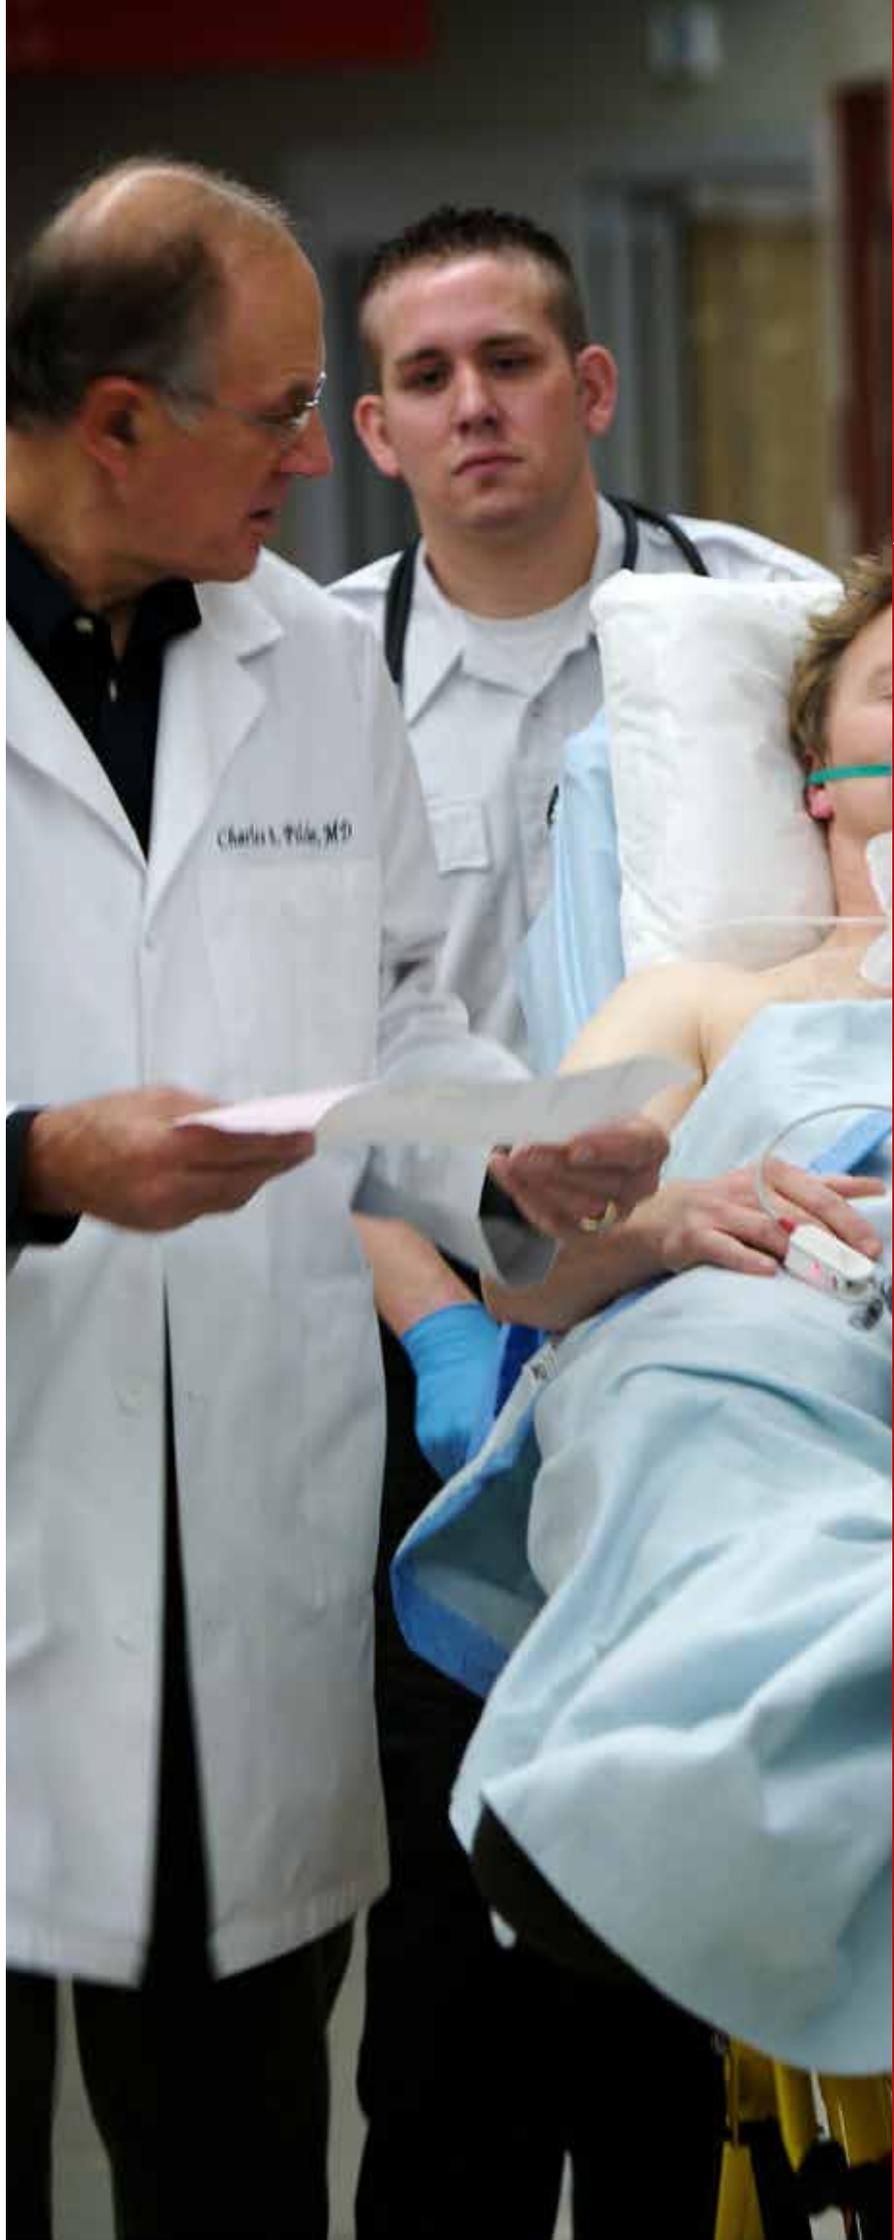

The standard in operational effectiveness.

Flexible, connected and easy to use, the LIFEPAK 15 monitor/defibrillator was designed based on the feedback and needs of people like you.

Upgradable platform

All LIFEPAK products are built as platforms, which means they are flexible enough to adapt to evolving protocols and new guidelines, and can be upgraded as you're ready to deliver new therapies. With more processing power and speed, the 15 is designed to grow as your needs change, helping you avoid costly premature replacements.

Flexible power options

Choose between external worldwide AC or DC power, or use the latest Lithium-ion dual battery technology for up to six hours of power. The LIFEPAK 15 monitor's two-battery system requires no maintenance or conditioning, and allows you to charge batteries in the device.

Data connectivity

The 15 collects code summaries and equipment status data along with critical clinical information as you treat patients. Using LIFENET Connect, part of the LIFENET System data network, the code summaries can be sent directly to your quality improvement team for review with CODE-STAT Data Review Software. Your equipment manager can also view equipment status on the LIFENET System using LIFENET Asset and alert you to any potential issues.

Attention to detail

The LIFEPAK15 device is designed for easy, intuitive use, which you can see through finishing touches such as an ergonomic handle, larger SPEED DIAL for easy selection, and an easy-to-clean keypad.

Dual-mode LCD screen with SunVue™ display

Switch from full-color to high-contrast SunVue mode with a single touch for the best full-glare view in the industry. A large screen (8.4 inches diagonally) and full-color display provide maximum viewability from all angles.

The standard in toughness.

The 15 is LIFEPAK TOUGH,[™] with improved ruggedness, portability and durability you can rely on.

Toughened inside and out

We heard from medical professionals that they wanted a more durable device—so we added a shock-absorbing handle, a double-layer screen that can withstand severe bumps and falls, and redesigned cable connections that lock tight for confident monitoring and therapy delivery. The 15 is the only device rated to withstand a 30" fall from bed height or a drop in transit.

Easy to clean

Industry-leading IP44 rating protects against fluids and substances, and exterior case and keypads are designed to help you meet requirements.

Unmatched field service

The unit's self-checking feature alerts our service team if the device needs attention, so you know it's ready when you need it. Our onsite maintenance and repair, access to original manufacturer parts, and highly trained, experienced service representatives give you the peace of mind that your LIFEPAK 15 will be ready when you need it.*



AC Power Adapter



LIFEPAK TOUGH[™]



CODE SUMMARY[™] critical event record


* A variety of customized service options are available.

LIFEPAK 15 MONITOR/DEFIBRILLATOR

The latest Lithium-ion battery technology and dual battery system allows for nearly six hour run time, automatic switching between external power and batteries, and an approximate two-year replacement cycle.

ST-Trend Tracking and 12-lead ECG transmissions via the LIFENET System makes the LIFEPAK 15 monitor/defibrillator a vital part of decreasing Door-to-Balloon (D2B) response times.

Integrated SpO₂, Carbon Monoxide, Methemoglobin, and temperature monitoring integrated into the device.

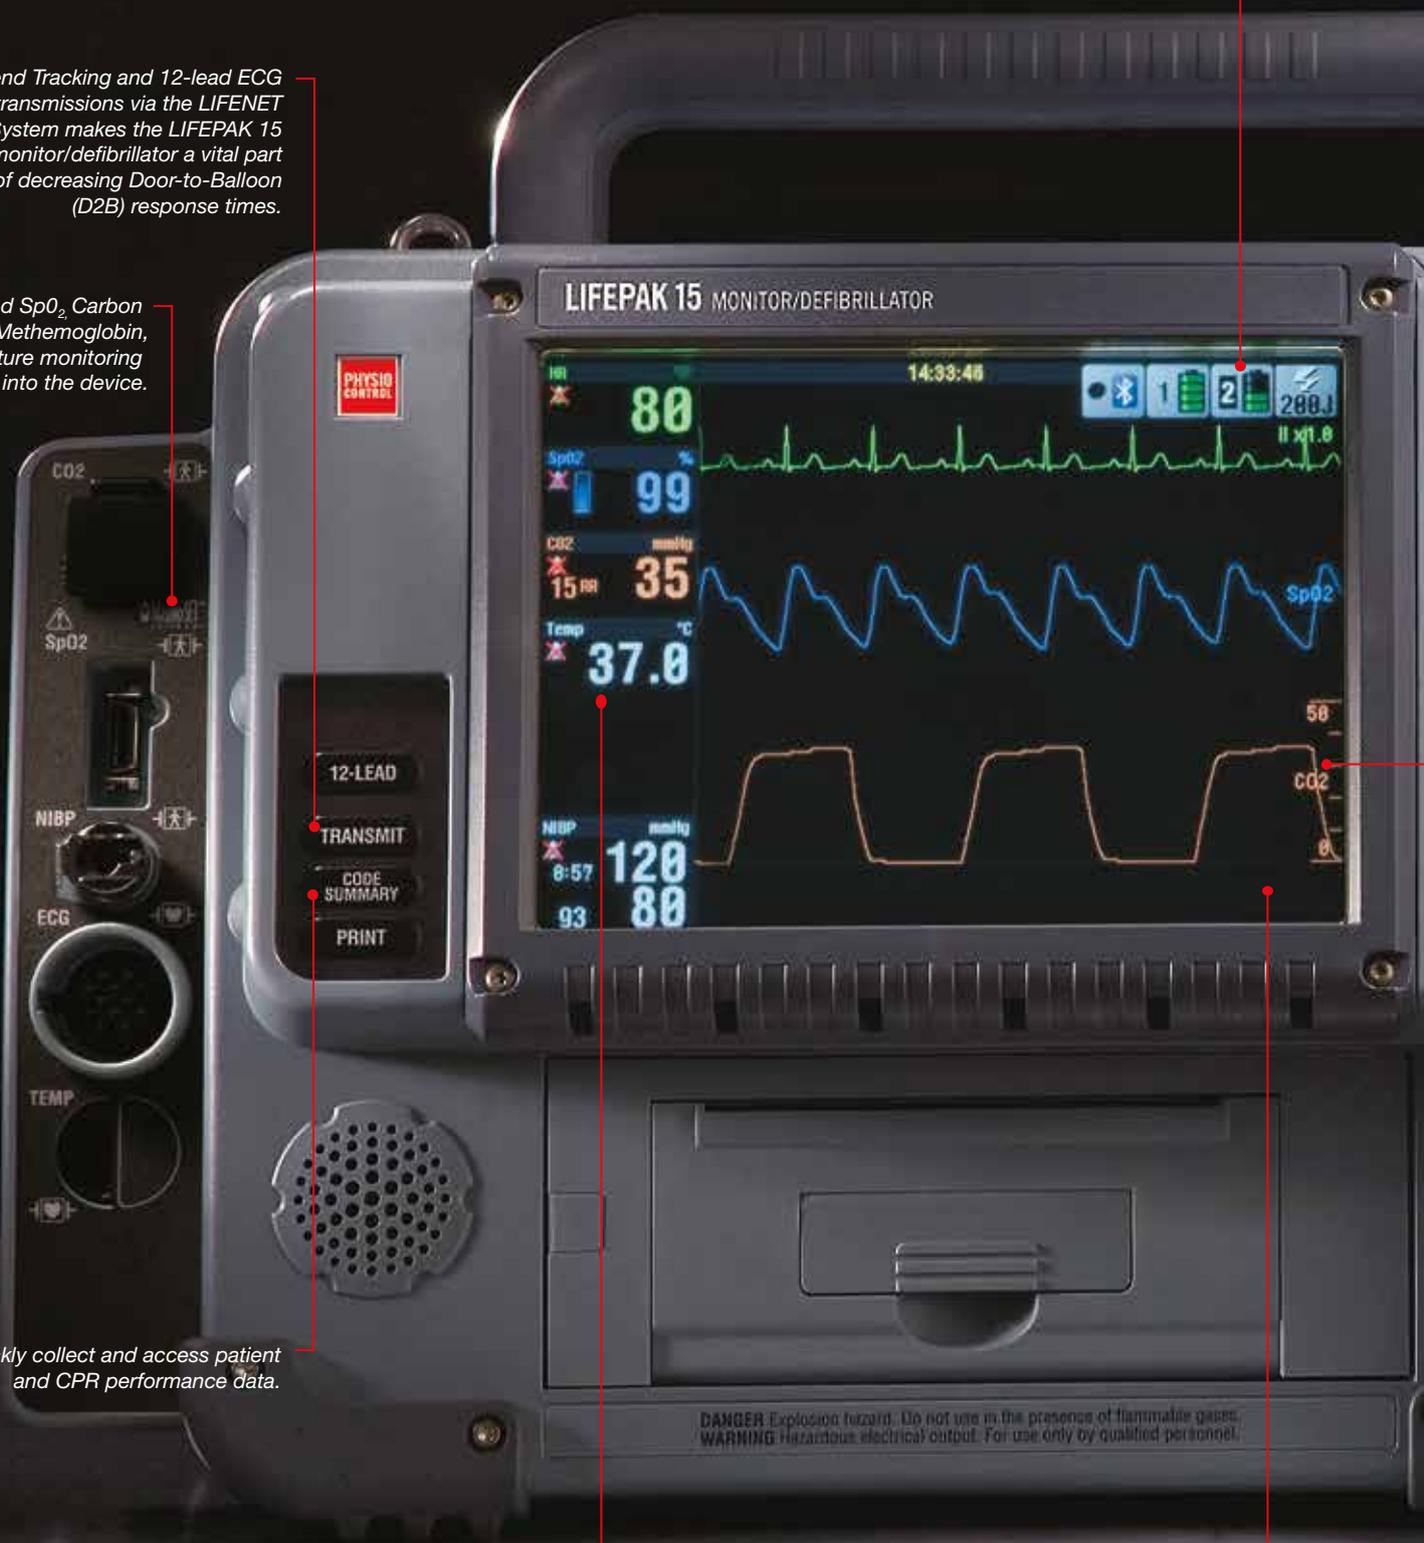


Quickly collect and access patient and CPR performance data.

On-screen temperature display in either Celsius or Fahrenheit.

Large screen with high resolution for maximum viewability in any setting.

Ergonomically designed handle has built-in shock absorbers for cushion and fits two gloved hands for easy pass off.

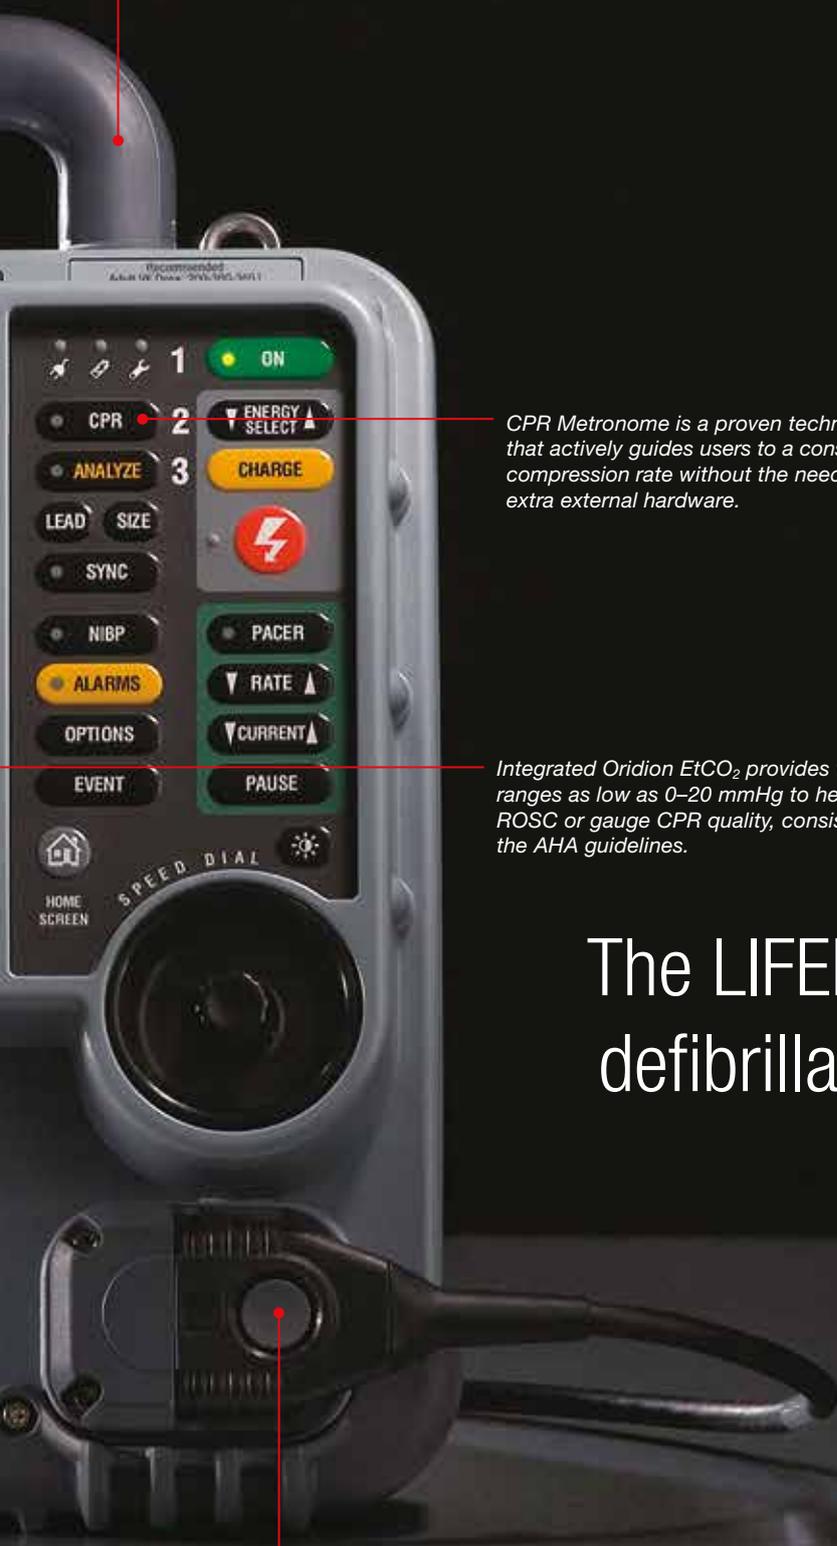

CPR Metronome is a proven technology that actively guides users to a consistent compression rate without the need for extra external hardware.

Integrated Oridion EtCO₂ provides waveform ranges as low as 0–20 mmHg to help identify ROSC or gauge CPR quality, consistent with the AHA guidelines.

The LIFEPAK 15 monitor/ defibrillator at a glance.

Redesigned cable connector gives you the confidence for secure therapy delivery.

A female healthcare professional with long brown hair, wearing blue scrubs and a stethoscope, is pushing a cart in a hospital hallway. The cart is carrying a LIFEPAK 15 monitor/defibrillator. The background shows a typical hospital corridor with white walls and doors.

For more than 60 years, Physio-Control has been developing technologies and designing devices that are legendary among first response professionals, clinical care providers and the community.

A legacy of trust.

Since we were founded in 1955, Physio-Control has been giving medical professionals around the world legendary quality and constant innovation. Our LIFEPAK devices have been carried to the top of Mount Everest. They've been launched into orbit on the International Space Station. And you'll find more than half a million units in use today on fire rescue rigs, ambulances and hospital crash carts worldwide.

We are inspired and informed by the rescuers who choose our products to save lives. The knowledge gained from working with some of the world's largest EMS organizations helps us constantly improve clinical standards and durability.

Today, we continue our legacy of innovation with leading technologies that improve patient care. Our 360J biphasic technology gives patients the best chance at survival. Our secure, web-based flow of ECG data helps improve STEMI patient outcomes. And our carbon monoxide monitoring helps catch the number one cause of poisoning deaths.

From the streets to the emergency room to the administrative office, we offer a full suite of solutions that range from code response to quality control analysis. And even as we bring ground-breaking products to the market, some things don't change. As always, when you choose our products, you don't just get a device. You also get the most comprehensive warranty in the business, industry-leading technical service, and a partner with over 60 years of experience in emergency care.

For more information about the LIFEPAK 15 monitor/defibrillator—and how it can help you do what you do best—please contact your local Physio-Control representative or visit www.physio-control.com.

Physio-Control Family of Products

Defibrillators/Monitors



LIFEPAK CR[®] Plus Automated External Defibrillator

Featuring the same advanced technology trusted by emergency medical professionals—yet simple to use—the fully automatic LIFEPAK CR Plus AED is designed specifically for the first person to respond to a victim of sudden cardiac arrest.



LIFEPAK[®] 1000 Defibrillator

The LIFEPAK 1000 Defibrillator is a powerful and compact device designed to treat cardiac arrest patients and provide continuous cardiac monitoring capabilities. Built-in flexibility allows the 1000 to be programmed for use by first responders or professionals and enables care providers to change protocols as standards of care evolve.



LIFEPAK[®] 15 Monitor/Defibrillator

The LIFEPAK 15 monitor/defibrillator is the standard in emergency care for ALS teams who want the most clinically innovative, operationally effective and LIFEPAK TOUGH™ device available today. The 15 offers sophisticated clinical technologies with a rich array of features—like the most powerful escalating energy available (up to 360J), advanced monitoring parameters and a completely upgradable platform.



LIFEPAK[®] 20e Defibrillator/Monitor with CodeManagement Module[®]

Clinically advanced and packed with power, the LIFEPAK 20e defibrillator/monitor is highly intuitive for first responders, and also skillfully combines AED function with manual capability so that ACLS-trained clinicians can quickly and easily deliver advanced therapeutic care. The CodeManagement Module adds waveform capnography and wireless connectivity to enhance your hospital's ability to effectively manage resuscitations from preparedness through review.

CPR Assistance



LUCAS[®] 2 Chest Compression System

Designed to provide effective, consistent and uninterrupted compressions according to AHA Guidelines, LUCAS can be used on adult patients in out-of-hospital and hospital settings.



TrueCPR™ Coaching Device

TrueCPR helps your team optimize their manual CPR performance using simple real-time and post-event feedback on the most critical resuscitation parameters. It accurately measures compression depth through proprietary Triaxial Field Induction technology.

Data Solutions



LIFENET® System

The LIFENET System provides EMS and hospital care teams with reliable, quick access to clinical information through a secure, web-based platform, helping to improve patient care, flow and operational efficiency.

CODE-STAT™ Data Review Software

CODE-STAT data review software is a retrospective analysis tool that provides easy access to data, reports and post-event review.

HealthEMS®

HealthEMS is a remote-hosted field data collection, management and reporting software solution which is proven to help Fire and EMS providers improve patient care and financial performance. HealthEMS creates a two-way information flow which dramatically improves the accuracy and timeliness of information needed to support billing and clinical decision-making.



PulsePoint

PulsePoint Respond alerts CPR-trained bystanders about nearby sudden cardiac arrests in a public area. The app guides the responder to the public location of the incident using a map while also identifying nearby AEDs. Because the PulsePoint solution is integrated into the local dispatch center, alerts are only sent after 911 has been notified.

PulsePoint AED is an app designed to build a comprehensive registry of AEDs available for use during cardiac emergencies. AED submissions are verified by the local agency and then become available within the Respond app.

Support



Physio-Control Service

With a service plan from Physio-Control, you are free to focus on your mission while relying on us to help to ensure the integrity of your lifesaving tools. From emergency repairs to software updates to preventive maintenance, we respond to every service call with speed and expertise so you have the peace of mind to do your job with confidence.

LIFEPAK 15 MONITOR/DEFIBRILLATOR



LIFEPAK 15 MONITOR

PHYSIO
CONTROL

160

SpO2 %
99

CO2 mmHg
15 RR 70



Temp °C
37.0

12-LEAD

TRANSMIT

CODE
SUMMARY

PRINT

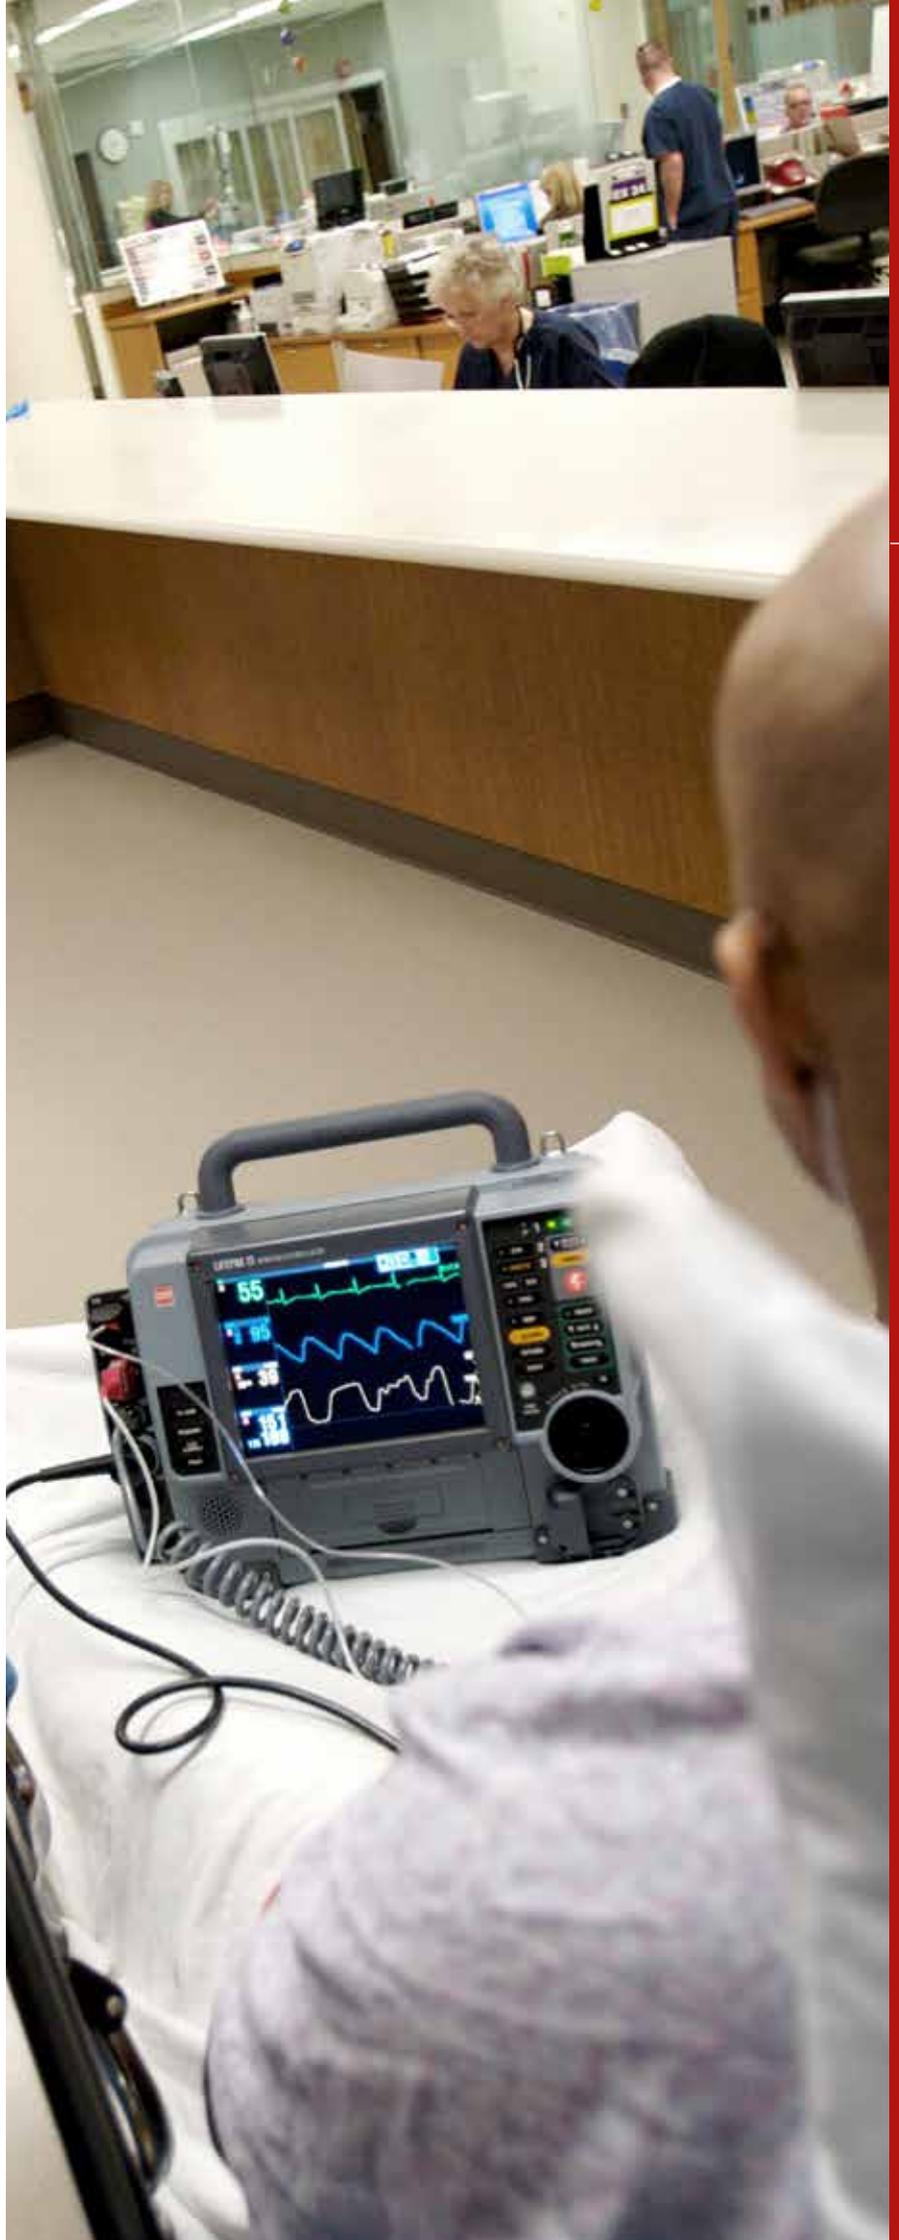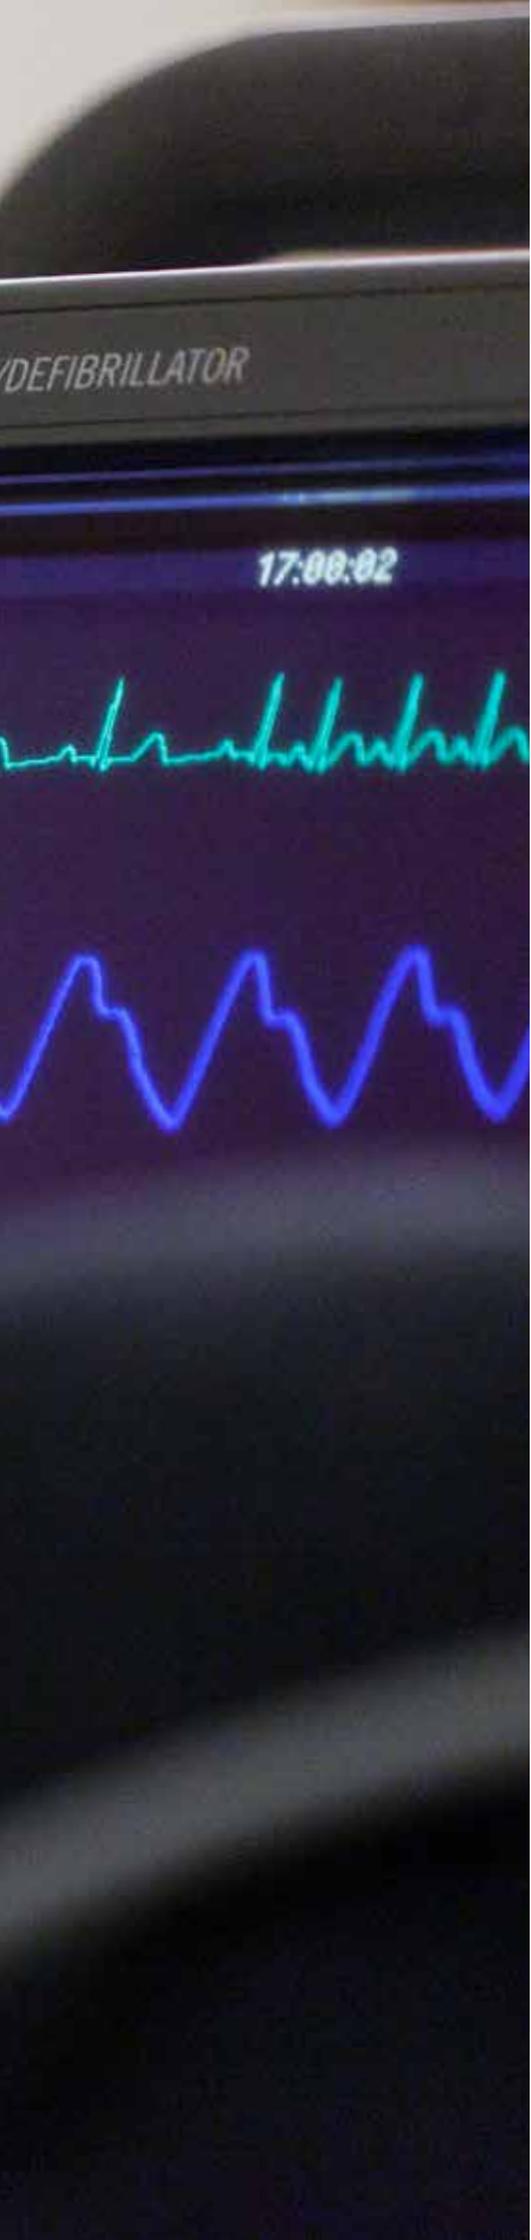

SPECIFICATIONS

GENERAL

The LIFEPAK 15 monitor/defibrillator has six main operating modes:

AED Mode: for automated ECG analysis and a prompted treatment protocol for patients in cardiac arrest.

Manual Mode: for performing manual defibrillation, synchronized cardioversion, noninvasive pacing, and ECG and vital sign monitoring.

Archive Mode: for accessing stored patient information.

Setup Mode: for changing default settings of the operating functions.

Service Mode: for authorized personnel to perform diagnostic tests and calibrations.

Demo Mode: for simulated waveforms and trend graphs for demonstration purposes.

PHYSICAL CHARACTERISTICS

Weight:

Basic monitor/defibrillator with new roll paper and two batteries installed: 7.9 kg (17.5 lb)

Fully featured monitor/defibrillator with new roll paper and two batteries installed: 8.4 kg (18.5 lb)

Lithium-ion battery: < 0.60 kg (1.3 lb)

Accessory Bags and Shoulder Strap: 1.77 kg (3.9 lb)

Standard (hard) Paddles: 0.95 kg (2.1 lb)

Height: 31.7 cm (12.5 in)

Width: 40.1 cm (15.8 in)

Depth: 23.1 cm (9.1 in)

DISPLAY

Size (active viewing area): 212 mm (8.4 in) diagonal; 171 mm (6.7 in) wide x 128 mm (5.0 in) high

Resolution: display type 640 dot x 480 dot color backlit LCD

User Selectable Display Mode: full color or SunVue™ display high contrast

Display: a minimum of 5 seconds of ECG and alphanumeric for values, device instructions, or prompts

Display: up to three waveforms

Waveform Display Sweep Speed: 25 mm/sec for ECG, SpO₂, IP, and 12.5 mm/sec for CO₂

DATA MANAGEMENT

The device captures and stores patient data, events (including waveforms and annotations), and continuous waveform and patient impedance records in internal memory.

The user can select and print reports, and transfer the stored information via supported communication methods.

Report Types:

- Three format types of CODE SUMMARY™ critical event record: short, medium, and long
- 12-lead ECG with STEMI statements
- Continuous Waveform (transfer only)
- Trend Summary
- Vital Sign Summary
- Snapshot

Memory Capacity: Total capacity is 360 minutes of continuous ECG, 90 minutes of continuous data from all channels, or 400 single waveform events.

Maximum memory capacity for a single patient includes up to 200 single waveform reports and 90 minutes of continuous ECG.

COMMUNICATIONS

The device is capable of transferring data records by wired or wireless connection. This device complies with Part 15 of the FCC rules, and its operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Serial Port RS232 communication + 12V available

Limited to devices drawing maximum 0.5 A current

Bluetooth® technology provides short-range wireless communication with other Bluetooth-enabled devices

MONITOR

ECG

ECG is monitored via several cable arrangements:

A 3-wire cable is used for 3-lead ECG monitoring.

A 5-wire cable is used for 7-lead ECG monitoring.

A 10-wire cable is used for 12-lead ECG acquisition. When the chest electrodes are removed, the 10-wire cable functions as a 4-wire cable.

Standard paddles or QUIK-COMBO® pacing/defibrillation/ECG electrodes are used for paddles lead monitoring.

Frequency Response:

Monitor: 0.5 to 40 Hz or 1 to 30 Hz

Paddles: 2.5 to 30 Hz

12-lead ECG diagnostic: 0.05 to 150 Hz

Lead Selection:

Leads I, II, III, (3-wire ECG cable)

Leads I, II, III, AVR, AVL, and AVF acquired simultaneously (4-wire ECG cable)

Leads I, II, III, AVR, AVL, AVF, and C lead acquired simultaneously (5-wire ECG cable)

Leads I, II, III, AVR, AVL, AVF, V1, V2, V3, V4, V5, and V6 acquired simultaneously (10-wire ECG cable)

ECG size: 4, 3, 2.5, 2, 1.5, 1, 0.5, 0.25 cm/mV (fixed at 1 cm/mV for 12-lead)

Heart Rate Display:

20–300 bpm digital display

Accuracy: ±4% or ±3 bpm, whichever is greater

QRS Detection Range Duration: 40 to 120 msec

Amplitude: 0.5 to 5.0 m

Common Mode Rejection (CMRR): ECG Leads: 90 dB at 50/60 Hz

SpO₂/SpCO/SpMet

Sensors:

MASIMO® sensors including RAINBOW® sensors

NELLCOR® sensors when used with the MASIMO RED™ MNC adapter

SpO₂

Displayed Saturation Range: “<50” for levels below 50%; 50 to 100%

Saturation Accuracy: 70–100% (0–69% unspecified)

Adults/Pediatrics:

±2 digits (during no motion conditions)

±3 digits (during motion conditions)

Dynamic signal strength bar graph

Pulse tone as SpO₂ pulsations are detected

SpO₂ Update Averaging Rate User selectable: 4, 8, 12 or 16 seconds

SpO₂ Sensitivity User selectable: Normal, High

SpO₂ Measurement: Functional SpO₂ values are displayed and stored

Pulse Rate Range: 25 to 240 bpm

Pulse Rate Accuracy (Adults/Pediatrics):

±3 digits (during no motion conditions)

±5 digits (during motion conditions)

Optional SpO₂ waveform display with autogain control

SpCO*

SpCO Concentration Display Range: 0 to 40%

SpCO Accuracy: ±3 digits

SpMET*

SpMet Saturation Range: 0 to 15.0%

SpMet Display Resolution: 0.1% up to 10%

SpMet Accuracy: ±1 digit

NIBP

Blood Pressure Systolic Pressure Range: 30 to 255 mmHg

Diastolic Pressure Range: 15 to 220 mmHg

Mean Arterial Pressure Range: 20 to 235 mmHg

Units: mmHg

Blood Pressure Accuracy: ±5 mmHg

Blood Pressure Measurement Time: 20 seconds, typical (excluding cuff inflation time)

Pulse Rate Range: 30 to 240 pulses per minute

Pulse Rate Accuracy: ±2 pulses per minute or ±2%, whichever is greater

Operation Features Initial Cuff Pressure: User selectable, 80 to 180 mmHg

Automatic Measurement Time Interval: User selectable, from 2 min to 60 min

Automatic Cuff Deflation Excessive Pressure: If cuff pressure exceeds 290 mmHg

Excessive Time: If measurement time exceeds 120 seconds

CO₂

CO₂ Range: 0 to 99 mmHg (0 to 13.2 kPa)

Units: mmHg, %, or kPa

Respiration Rate Accuracy:

0 to 70 bpm: ±1 bpm

71 to 99 bpm: ±2 bpm

Respiration Rate Range: 0 to 99 breaths/minute

Rise Time: 190 msec

Response Time: 3.3 seconds (includes delay time and rise time)

Initialization Time: 30 seconds (typical), 10–180 seconds

Ambient Pressure: automatically compensated internally

Optional Display: CO₂ pressure waveform

Scale factors: Autoscale, 0–20 mmHg (0–4 Vol%), 0–50 mmHg (0–7 Vol%), 0–100 mmHg (0–14 Vol%)

Invasive Pressure

Transducer Type: Strain-gauge resistive bridge

Transducer Sensitivity: 5µV/V/mmHg

Excitation Voltage: 5 Vdc

Connector: Electro Shield: CXS 3102A 14S-6S

Bandwidth: Digital filtered, DC to 30 Hz (< -3db)

Zero Drift: 1 mmHg/hr without transducer drift

Zero Adjustment: ±150 mmHg including transducer offset

Numeric Accuracy: ±1 mmHg or 2% of reading, whichever is greater, plus transducer error

Pressure Range: -30 to 300 mmHg, in six user selectable ranges

Invasive Pressure Display

Display: IP waveform and numerics

Units: mmHg

Labels: P1 or P2, ART, PA, CVP, ICP, LAP (user selectable)

Temperature

Range: 24.8° to 45.2°C (76.6° to 113.4°F)

Resolution: 0.1°C

Accuracy: ±0.2°C including sensor

Reusable Temperature Cable: 5 foot or 10 foot

Disposable Sensor Types: Surface–Skin; Esophageal/Rectal

Trend

Time Scale: Auto, 30 minutes, 1, 2, 4, or 8 hours

Duration: Up to 8 hours

ST Segment: After initial 12-lead ECG analysis, automatically selects and trends ECG lead with the greatest ST displacement

Display Choice of: HR, PR (SpO₂), PR (NIBP), SpO₂ (%), SpCO (%), SpMet (%), CO₂ (ETCO₂/FICO₂), RR (CO₂), NIBP, IP1, IP2, ST

ALARMS

Quick Set: Activates alarms for all active vital signs

VF/VT Alarm: Activates continuous (CPSS) monitoring in Manual mode

Apnea Alarm: Occurs when 30 seconds has elapsed since last detected respiration

Heart Rate Alarm Limit Range: Upper, 100–250 bpm; lower, 30–150 bpm

INTERPRETIVE ALGORITHM

12-Lead Interpretive Algorithm: University of Glasgow

12-Lead ECG Analysis Program, includes AMI and STEMI statements

PRINTER

Prints continuous strip of the displayed patient information and reports

Paper Size: 100 mm (3.9 in)

Print Speed: 25 mm/sec or 12.5 mm/sec

Optional: 50 mm/sec time base for 12-lead ECG reports

Delay: 8 seconds

Autoprint: Waveform events print automatically

Frequency Response:

Diagnostic: 0.05 to 150 Hz or 0.05 to 40 Hz

Monitor: 0.67 to 40 Hz or 1 to 30 Hz

DEFIBRILLATOR

Biphasic Waveform: Biphasic Truncated Exponential

The following specifications apply from 25 to 200 ohms, unless otherwise specified:

Energy Accuracy: ±1 joule or 10% of setting, whichever is greater, into 50 ohms, ±2 joules or 15% of setting, whichever is greater, into 25-175 ohms.

Voltage Compensation: Active when disposable therapy electrodes are attached. Energy output within ±5% or ±1 joule, whichever is greater, of 50 ohms value, limited to the available energy which results in the delivery of 360 joules into 50 ohms.

Paddle Options: QUIK-COMBO pacing/defibrillation/ECG electrodes (standard). Cable Length 8 foot long (2.4 m) QUIK-COMBO cable (not including electrode assembly).

Standard paddles (optional)

Manual Mode

Energy Select: 2, 3, 4, 5, 6, 7, 8, 9, 10, 15, 20, 30, 50, 70, 100, 125, 150, 175, 200, 225, 250, 275, 300, 325, and 360 joules

Charge Time: Charge time to 360 joules in less than 10 seconds, typical

Synchronous Cardioversion: Energy transfer begins within 60 msec of the QRS peak

Paddles Lead Off Sensing: When using QUIK-COMBO electrodes, the device indicates Paddles Leads Off if the resistive part of the patient impedance is greater than 300 ±15% ohms, or if the magnitude of the patient impedance is greater than 440 ±15% ohms.

AED Mode

Shock Advisory System™ (SAS): an ECG analysis system that advises the operator if the algorithm detects a shockable or non-shockable ECG rhythm. SAS acquires ECG via therapy electrodes only.

Shock Ready Time: Using a fully charged battery at normal room temperature, the device is ready to shock within 20 seconds if the initial rhythm finding is "SHOCK ADVISED"

Biphasic Output: Energy Shock levels ranging from 150–360 joules with same or greater energy level for each successive shock

cprMAX™ Technology: In AED mode, cprMAX technology provides a method of maximizing the CPR time that a patient receives, with the overall goal of improving the rate of survival of patients treated with AEDs.

Setup Options:

– Auto Analyze: Allows for auto analysis. Options are OFF, AFTER 1ST SHOCK

– Initial CPR: Allows the user to be prompted for CPR for a period of time prior to other activity. Options are OFF, ANALYZE FIRST, CPR FIRST

– Initial CPR Time: Time interval for Initial CPR. Options are 15, 30, 45, 60, 90, 120, and 180 seconds.

– Pre-Shock CPR: Allows the user to be prompted for CPR while the device is charging. Options are OFF, 15, 30 seconds.

– Pulse Check: Allows the user to be prompted for a pulse check at various times. Options are ALWAYS, AFTER EVERY SECOND NSA, AFTER EVERY NSA, NEVER

– Stacked Shocks: Allows for CPR after 3 consecutive shocks or after a single shock. Options are OFF, ON

– CPR Time: 1 or 2 User selectable times for CPR. Options are 15, 30, 45, 60, 90, 120, 180 seconds and 30 minutes.

PACER

Pacing Mode: Demand or non-demand rate and current defaults

Pacing Rate: 40 to 170 PPM

Rate Accuracy: ±1.5% over entire range

Output Waveform: Monophasic, truncated exponential current pulse (20 ± 1 ms)

Output Current: 0 to 200 mA

Pause: Pacing pulse frequency reduced by a factor of 4 when activated

Refractory Period: 180 to 280 msec (function of rate)

ENVIRONMENTAL

Unit meets functional requirements during exposure to the following environments unless otherwise stated.

Operating Temperature: 0° to 45°C (32° to 113°F); -20°C (-4°F) for 1 hour after storage at room temperature; 60°C (140°F) for 1 hour after storage at room temperature

Storage Temperature: -20° to 65°C (-4° to 149°F) except therapy electrodes and batteries

Relative Humidity, Operating: 5 to 95%, non-condensing. NIBP: 15 to 95%, non-condensing

Relative Humidity, Storage: 10 to 95%, non-condensing

Atmospheric Pressure, Operating: -382 to 4,572 m (-1,253 to 15,000 ft). NIBP: -152 to 3,048 m (-500 to 10,000 ft)

Water Resistance, Operating: IP44 (splash proof, dust and sand resistant) per IEC 529 and EN 1789 (without accessories except for 12-lead ECG cable, hard paddles, and battery pack)

Vibration: MIL-STD-810E Method 514.4, Propeller Aircraft - category 4 (figure 514.4-7 spectrum a), Helicopter - category 6 (3.75 Grms), Ground Mobile - category 8 (3.14 Grms), EN 1789: Sinusoidal Sweep, 1 octave/min, 10-150 Hz, ±0.15 mm/2 g

Shock (drop): 5 drops on each side from 18 inches onto a steel surface EN 1789: 30-inch drop onto each of 6 surfaces

Shock (functional): Meets IEC 60068-2-27 and MIL-STD-810E shock requirements 3 shocks per face at 40 g, 6 ms half-sine pulses

Bump: 1000 bumps at 15 g with pulse duration of 6 msec

Impact, Non-operating: EN 60601-1 0.5 + 0.05 joule impact UL 60601-1 6.78 Nm impact with 2-inch diameter steel ball. Meets IEC62262 protection level IK 04.

EMC: EN 60601-1-2:2006 Medical Equipment - General Requirements for Safety - Collateral Standard: Electromagnetic Compatibility - Requirements and Tests EN 60601-2-4:2003: (Clause 36) Particular Requirements for the Safety of Cardiac Defibrillators and Cardiac Defibrillator-Monitors

Cleaning: Cleaning 20 times with the following: Quaternary ammonium, isopropyl alcohol, hydrogen peroxide

Chemical Resistance: 60 hour exposure to specified chemicals: Betadine (10% Povidone-Iodine solution), Coffee, Cola, Dextrose (5% Glucose solution), Electrode Gel/Paste (98% water, 2% Carbopol 940), HCL (0.5% solution, pH=1), Isopropyl Alcohol, NaCl solution (0.9% solution), Cosmetic discoloration of the paddle well shorting bar shall be allowed following exposure to HCL (0.5% solution).

POWER

Power Adapters: AC or DC

Power Adapters provide operation and battery charging from external AC or DC power

– Full functionality with or without batteries when connected to external AC/DC

– Typical battery charge time while installed in LIFEPAK 15 device is 190 minutes

– Indicators: external power indicator, battery charging indicator

Dual battery: Capability with automatic switching

Low battery indication and message: Low battery fuel gauge indication and low battery message in status area for each battery

Replace battery indication and message: Replace battery fuel gauge indication, audio tones and replace battery message in the status area for each battery. When replace battery is indicated, device auto-switches to second battery. When both batteries reach replace battery condition, a voice prompt instructs user to replace battery.

Battery Capacity For two, new fully-charged batteries, 20°C (68°F)

Operating Mode		Monitoring	Pacing	Defibrillation
		(minutes)	(minutes)	(360J discharges)
Total Capacity to Shutdown	Typical	360	340	420
	Minimum	340	320	400
Capacity After Low Battery	Typical	21	20	30
	Minimum	12	10	6

BATTERY

Battery Specifications

Battery Type: Lithium-ion

Weight: < 0.60 kg (1.3 lb)

Charge Time (with fully depleted battery): 4 hours and 15 minutes (typical)

Battery indicators: Each battery has a fuel gauge that indicates its approximate charge. A fuel gauge that shows two or fewer LEDs after a charge cycle indicates that the battery should be replaced.

Charging Temperature Range: 5° to 45°C (41° to 113°F)

Operating Temperature Range: 0° to 45°C (32° to 113°F)

Short Term (<1 week) Storage Temperature Range: -20° to 60°C (-4° to 140°F)

Long Term (>1 week) Storage Temperature Range: 20° to 25°C (68° to 77°F)

Operating and Storage Humidity Range: 5 to 95% relative humidity, non-condensing

REFERENCES

- 1 Stiel I, Walker R, Nesbitt L, et al. Biphasic Trial: A randomized comparison of fixed lower versus escalating higher energy levels for defibrillation in out-of-hospital cardiac arrest. *Circulation*. 2007;115:1511-1517.
- 2 Edelson D, Litzinger B, Arora V, et al. Improving in-hospital cardiac arrest process and outcomes with performance debriefing. *Arch Intern Med*. 2008;168:1063-1069.
- 3 Olasveengen T, Wik L, Kramer-Johansen J, et al. Is CPR quality improving? A retrospective study of out-of-hospital cardiac arrest. *Resuscitation*. 2007;75:260-266.
- 4 Fletcher D, Galloway R, Chamberlain D, et al. Basics in advanced life support: A role for download audit and metronome. *Resuscitation*. 2008;78:127-134.

All claims valid as of July 2015.

For further information please contact your local Physio-Control representative or visit our website at www.physio-control.com



Physio-Control Headquarters
11811 Willows Road NE
Redmond, WA 98052 USA
Tel 425 867 4000
Fax 425 867 4121
www.physio-control.com

**Physio-Control Operations
Netherlands B.V.**
HQ Europe, Middle East & Africa
UP Office Building
Piet Heinkade 55,
1019 GM Amsterdam NL
Tel +31 (0)20 7070560
Fax +31 (0)20 3391194
www.physio-control.com

**Physio-Control
UK Sales Ltd**
Concorde House
Trinity Park, Solihull
Birmingham
B37 7UQ
United Kingdom
Tel +44 (0)808 258 0094
Fax +44 (0)808 189 0337

**Physio-Control
Australia Pty Ltd**
Suite 4.01
15 Orion Road
Lane Cove
NSW 2066
Australia
Toll Free Tel 1800 987 982
Toll Free Fax 1800 890 892